

FIG. 1

1000324-10601

FIG. 2


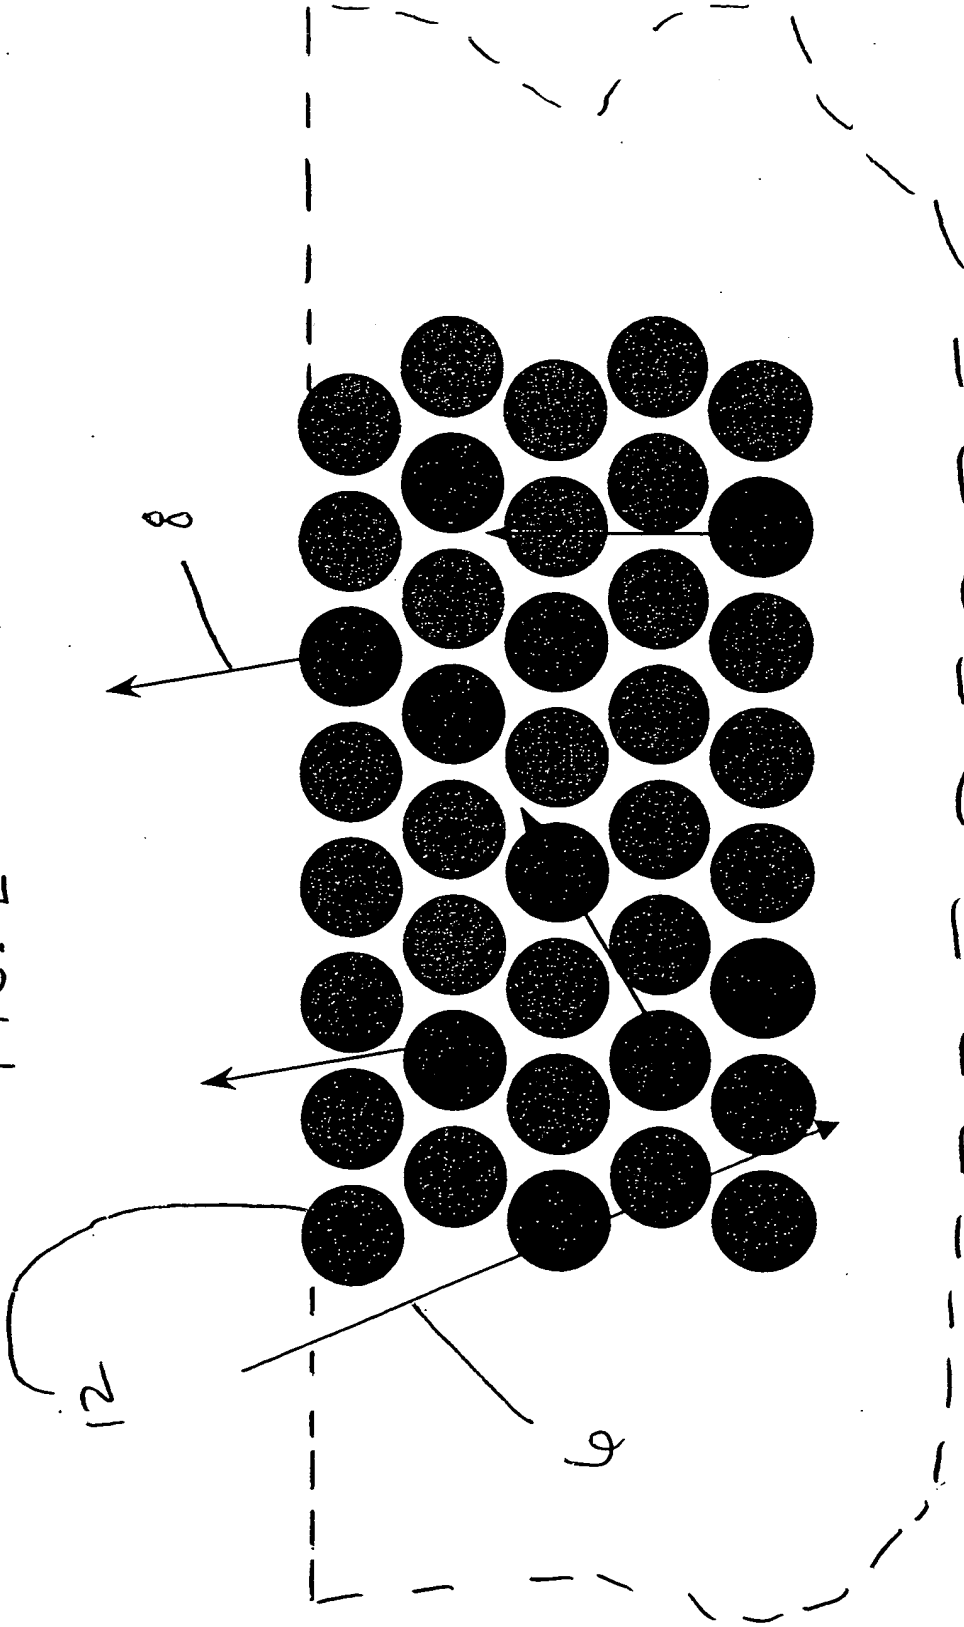


FIG. 3

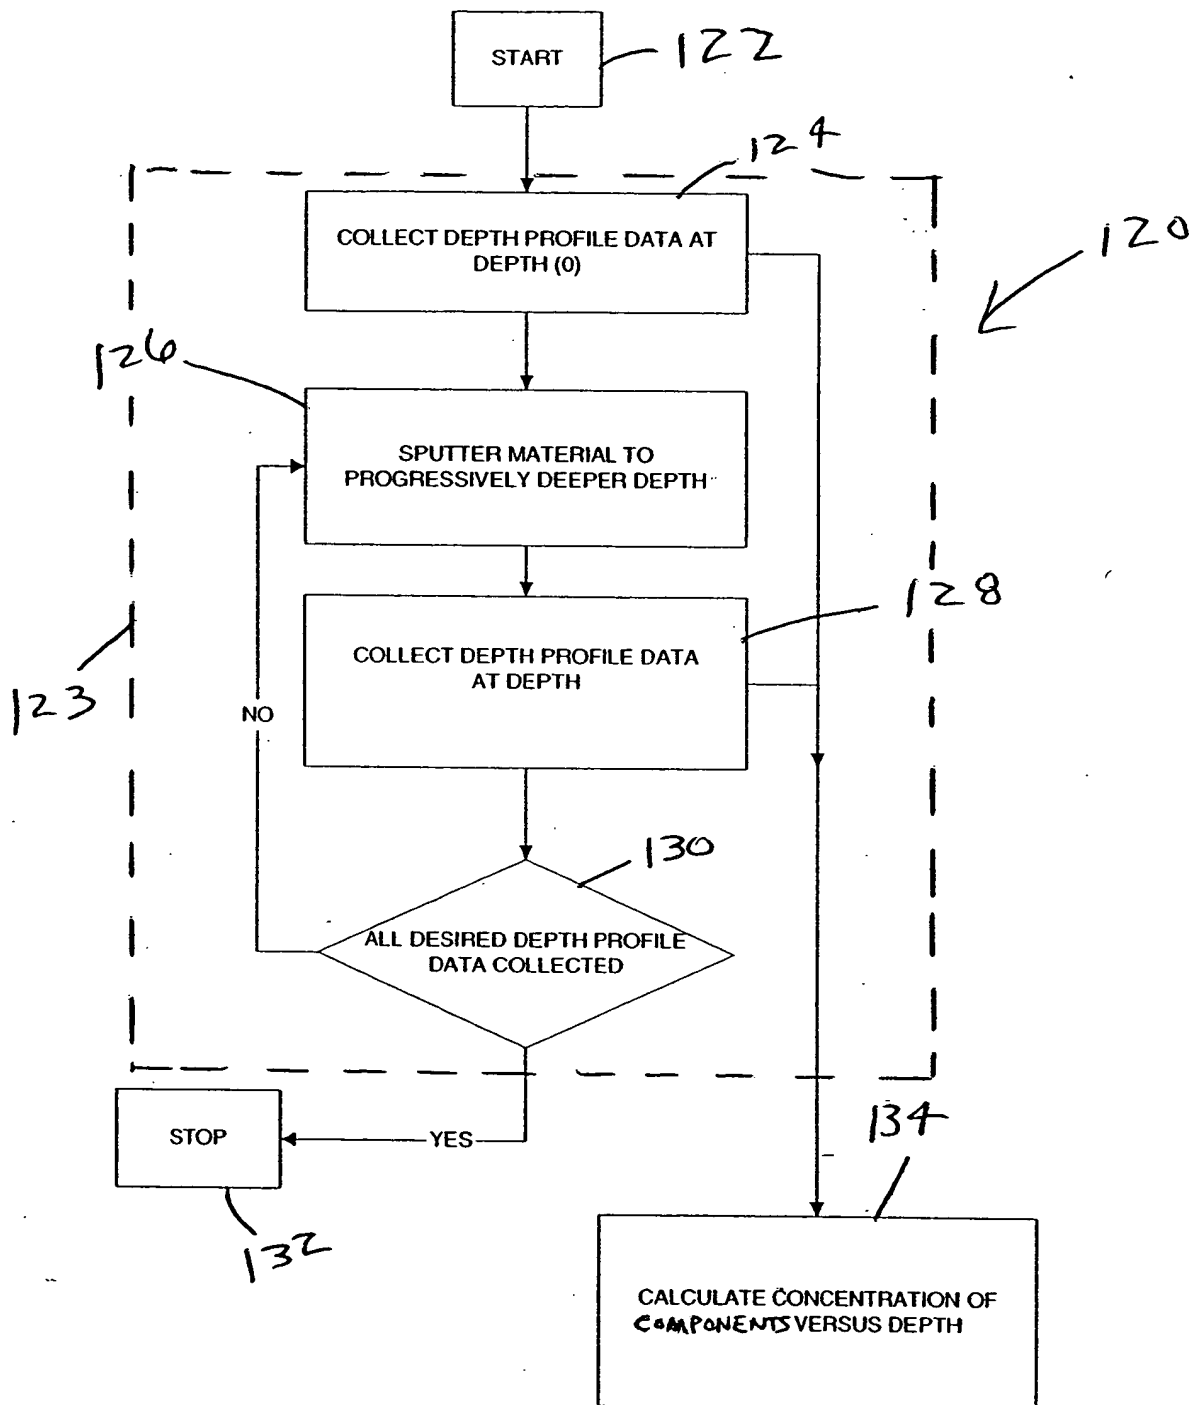

FO920T 422E000T

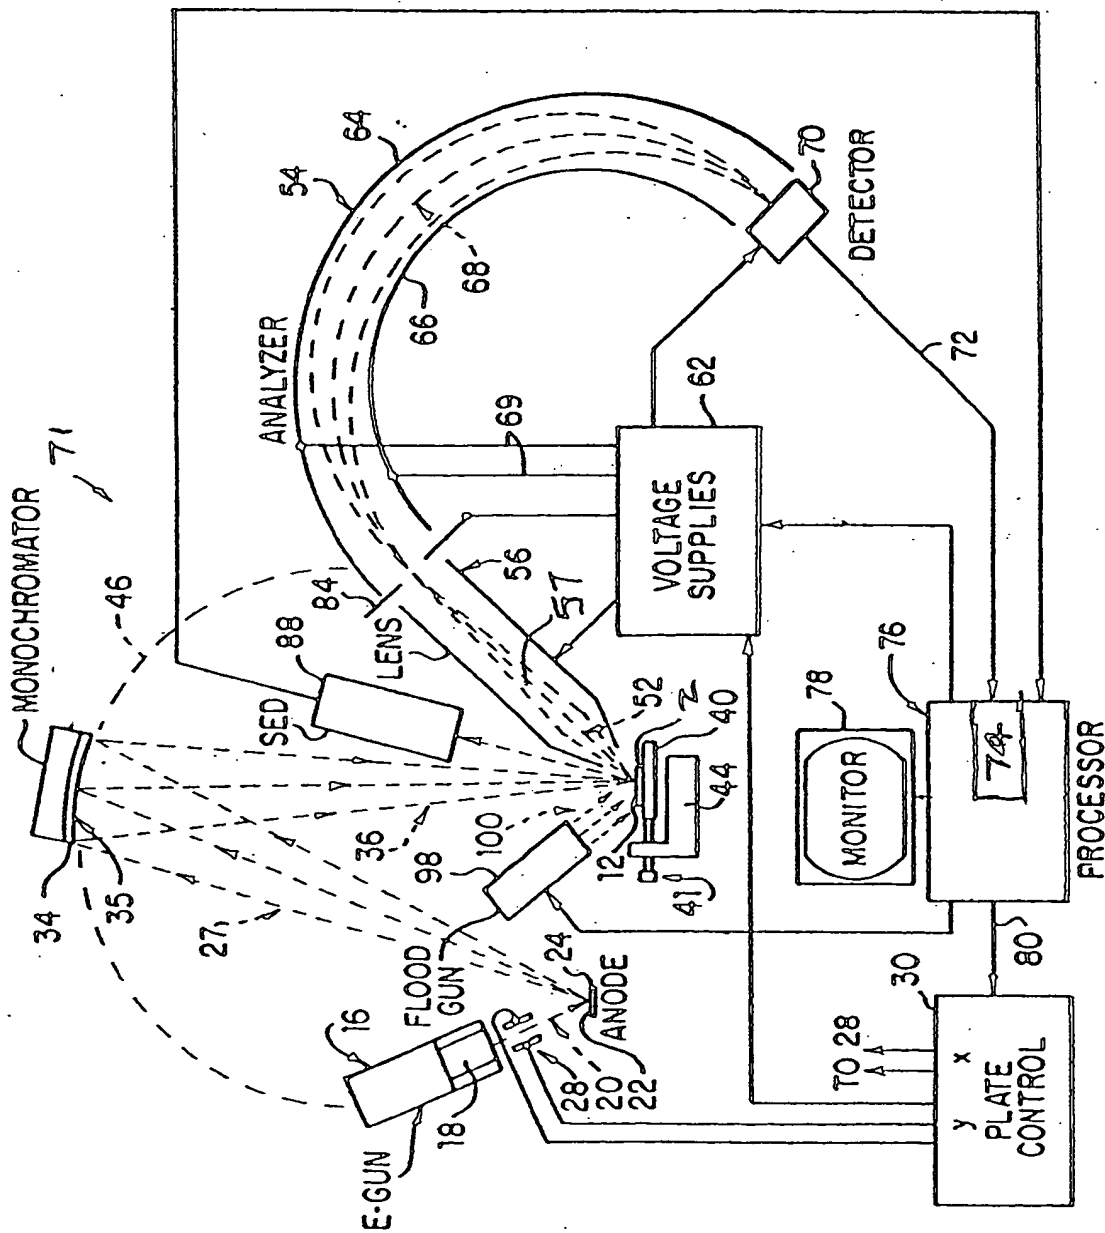


FIG. 5A


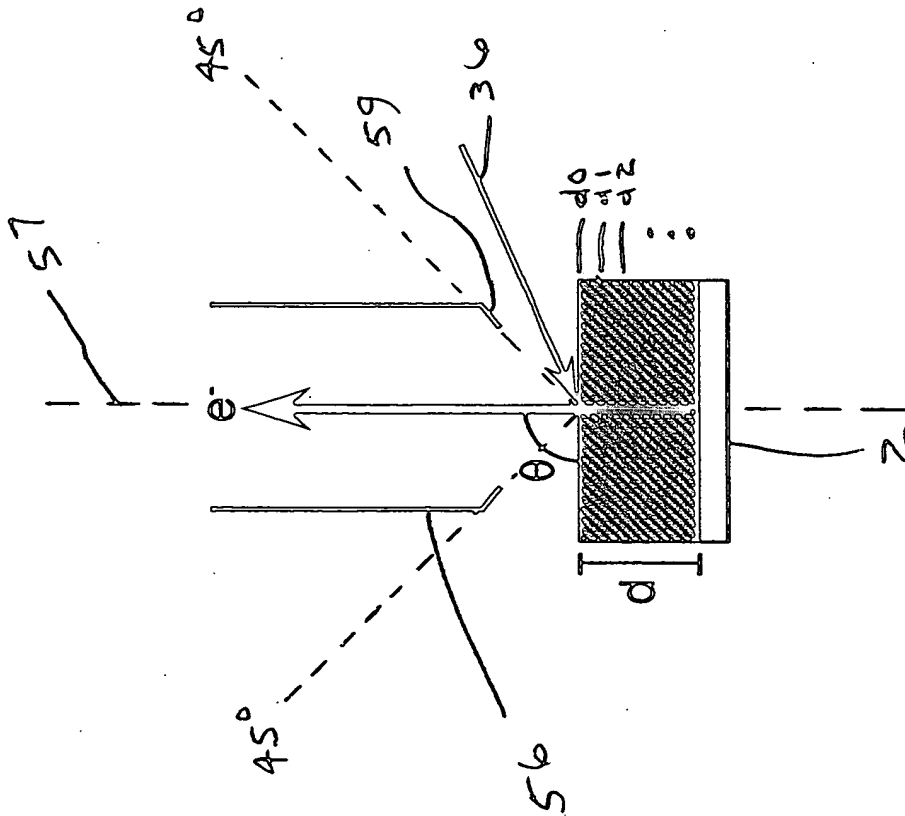


FIG. 5B

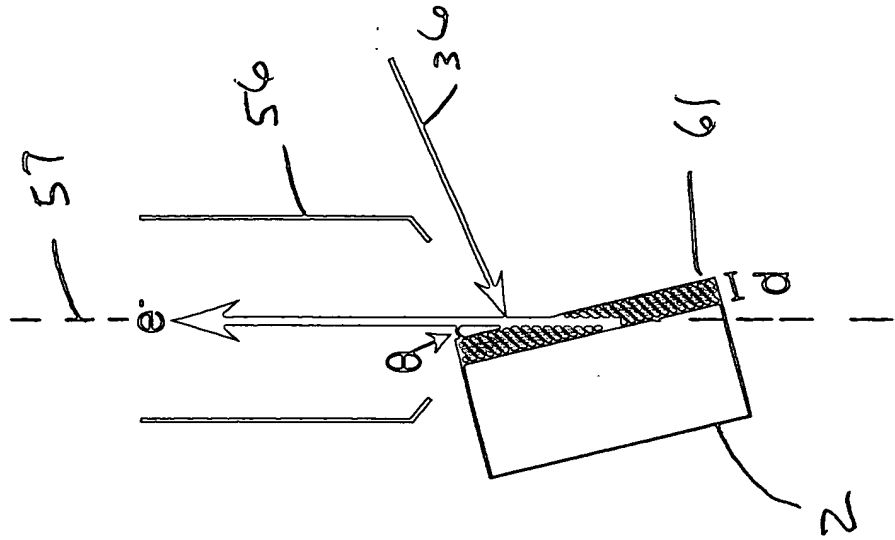

SCANNED # 24

FIG. 6

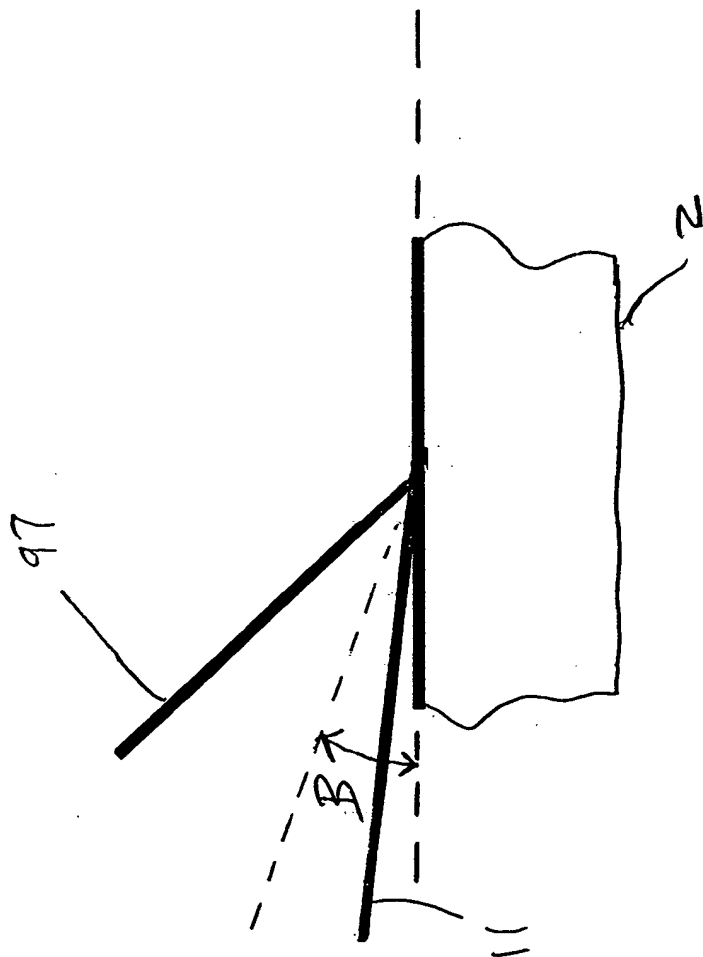


FIG. 7



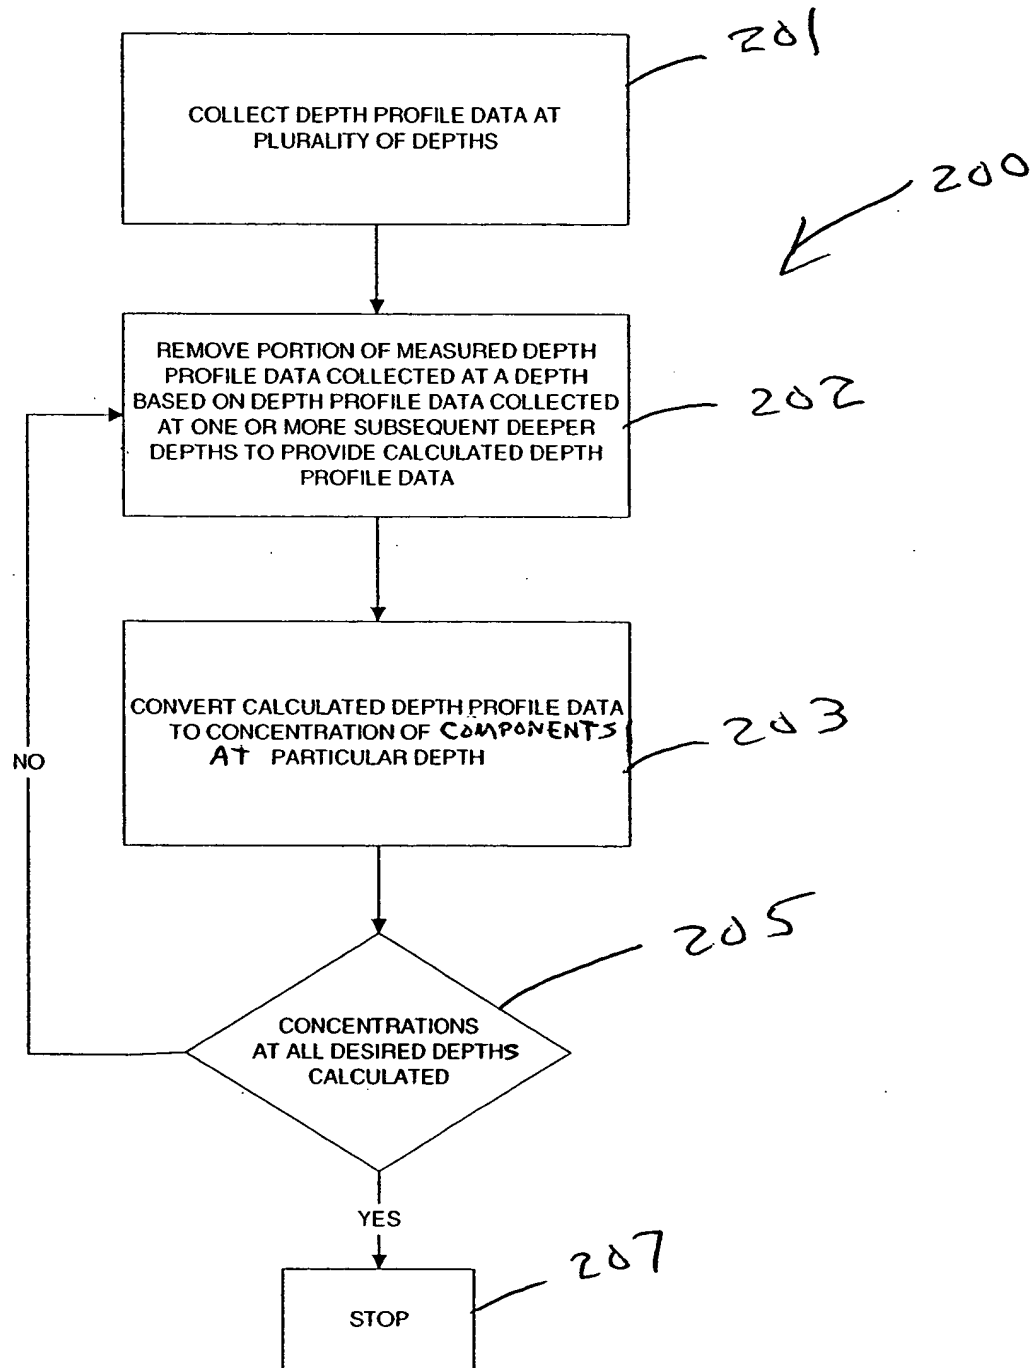


FIG. 8

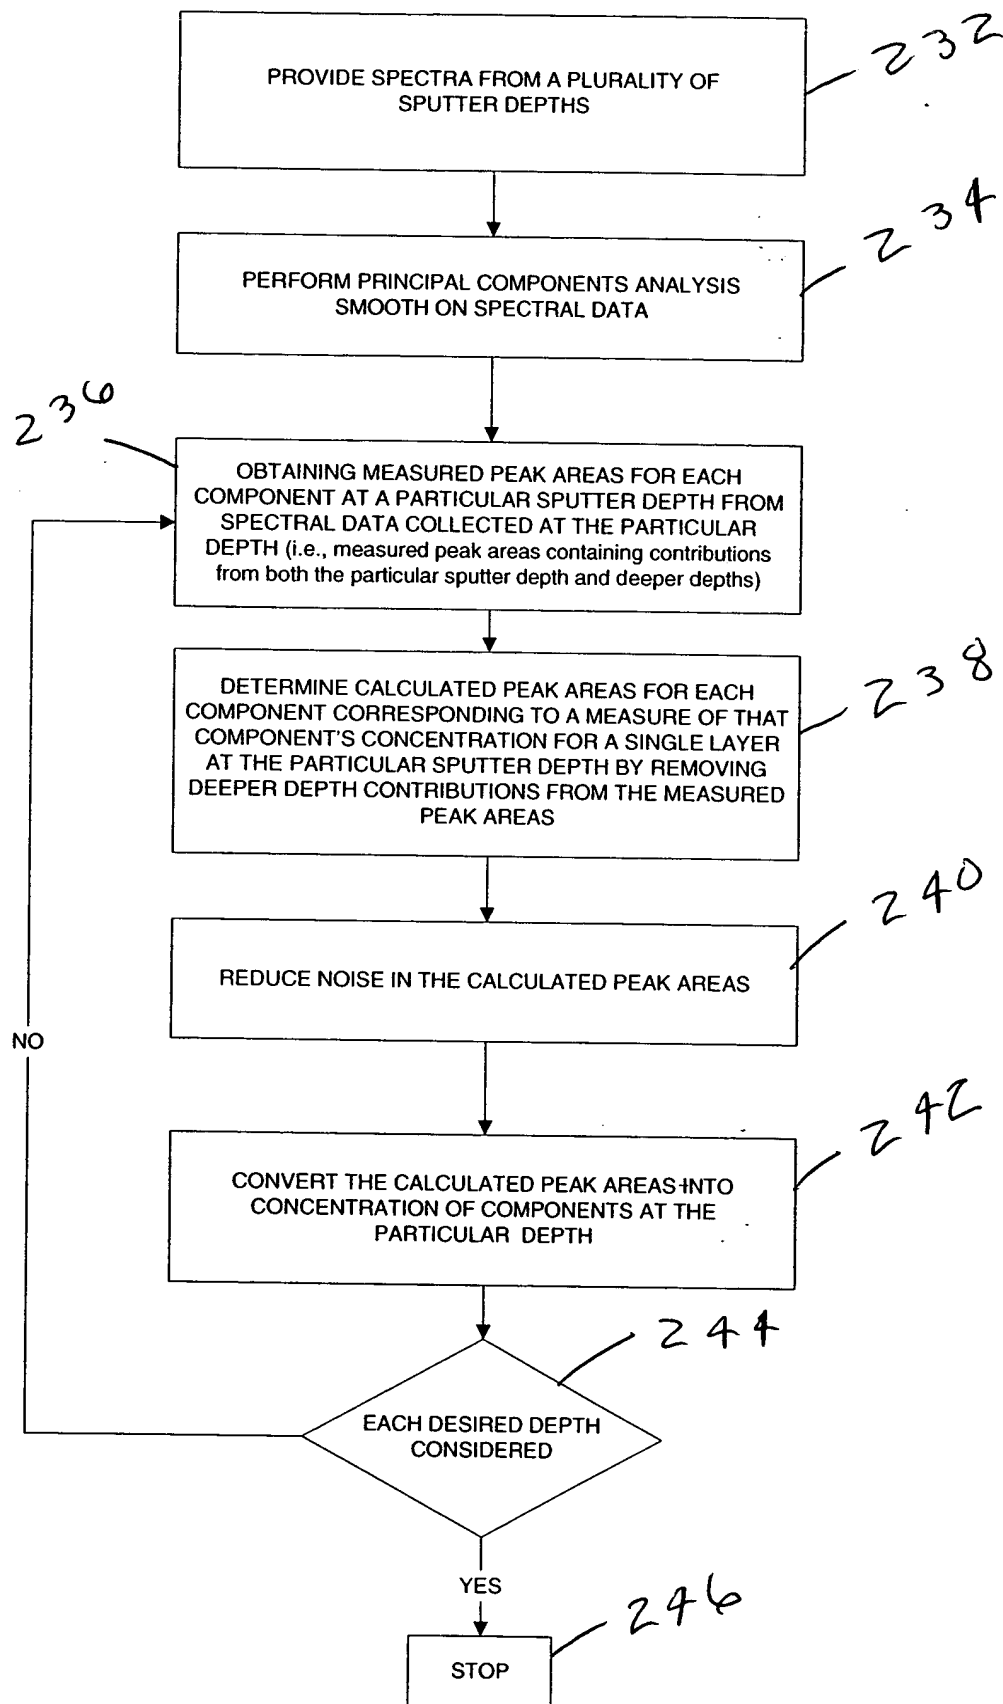


10003224.102601

FIG. 9

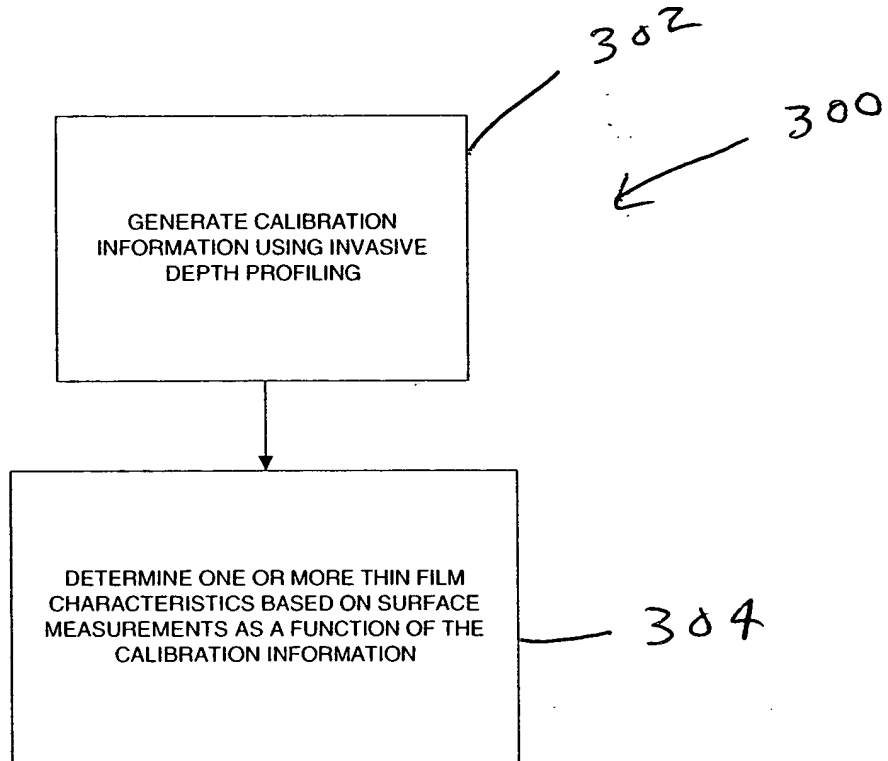


10003224.102601

FIG. 10

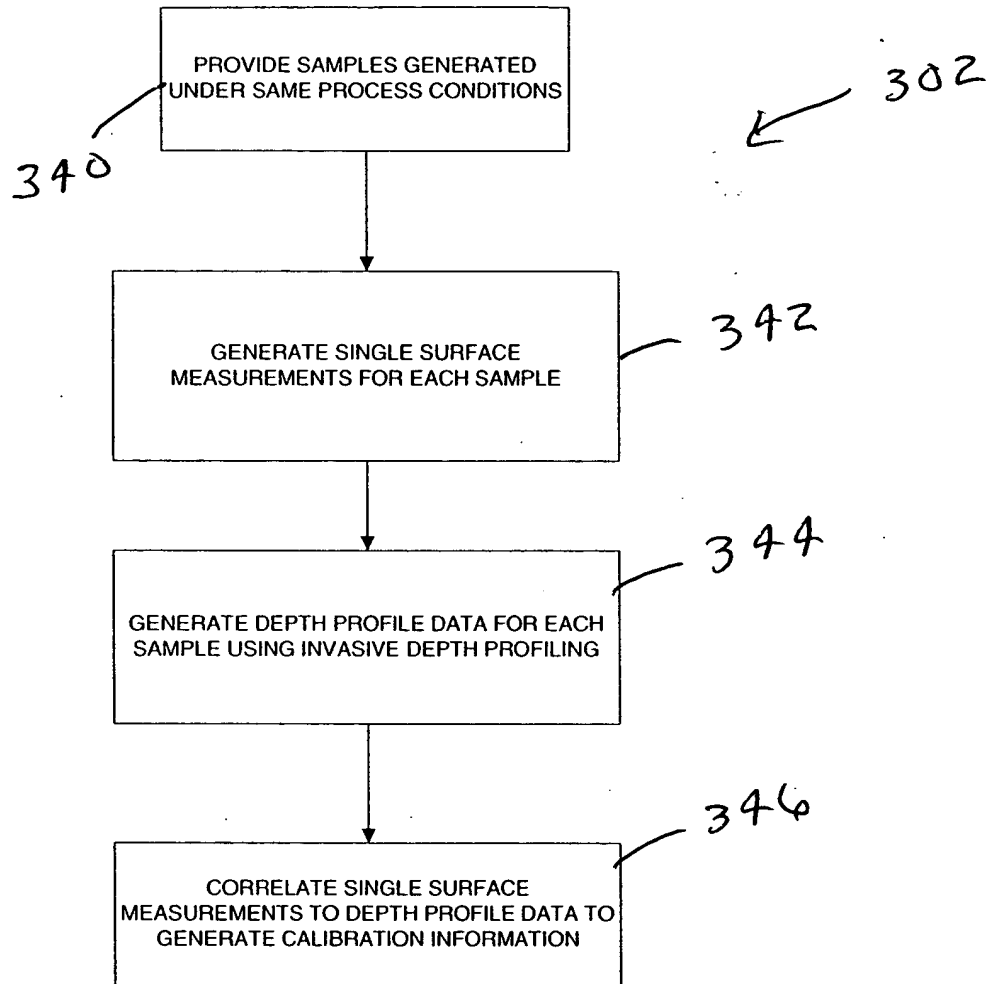

10003224-102601


FIG. 11

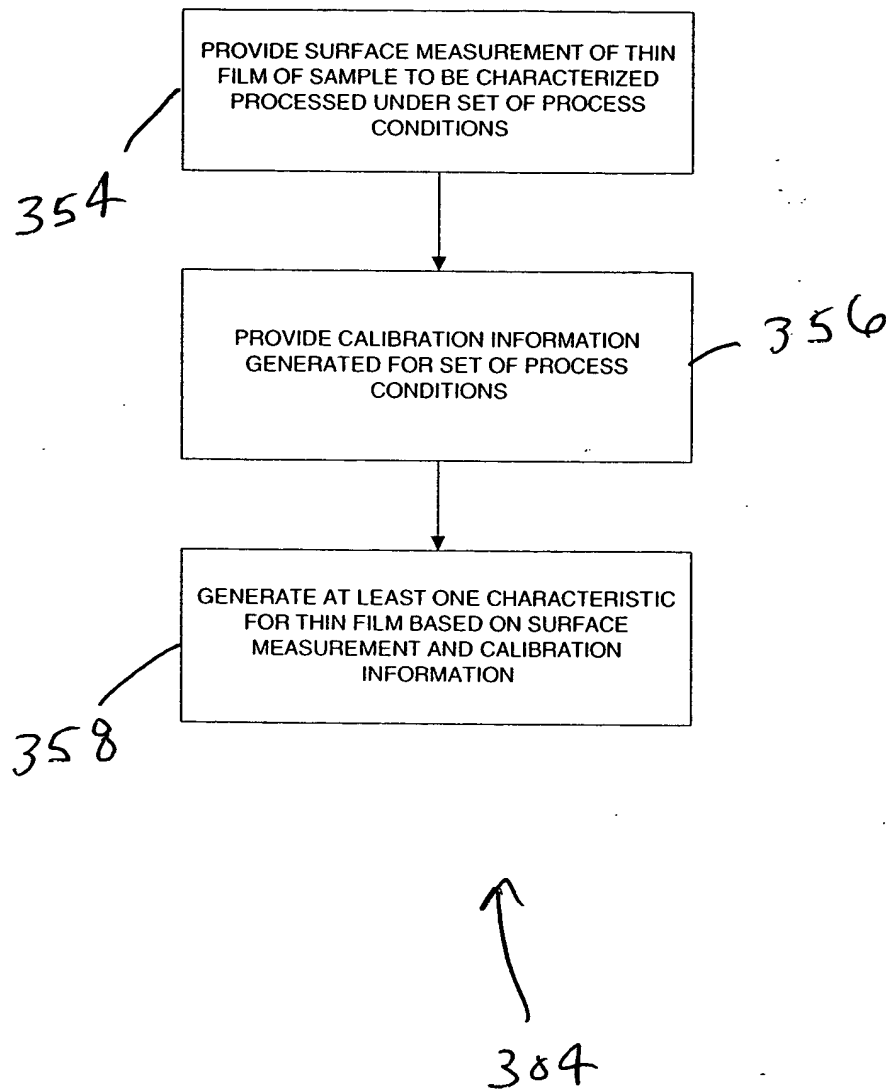

10003224.102601

FIG. 12

(single measurement)

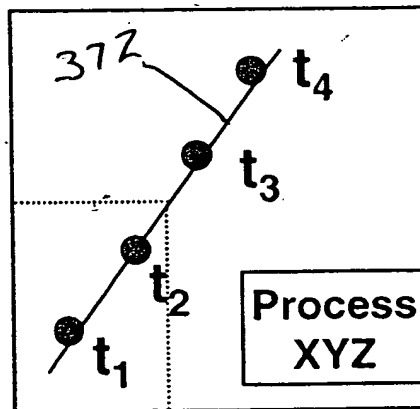


Total N Dose
(calibration with
depth profile)

370


1000324-102501

FIG. 13

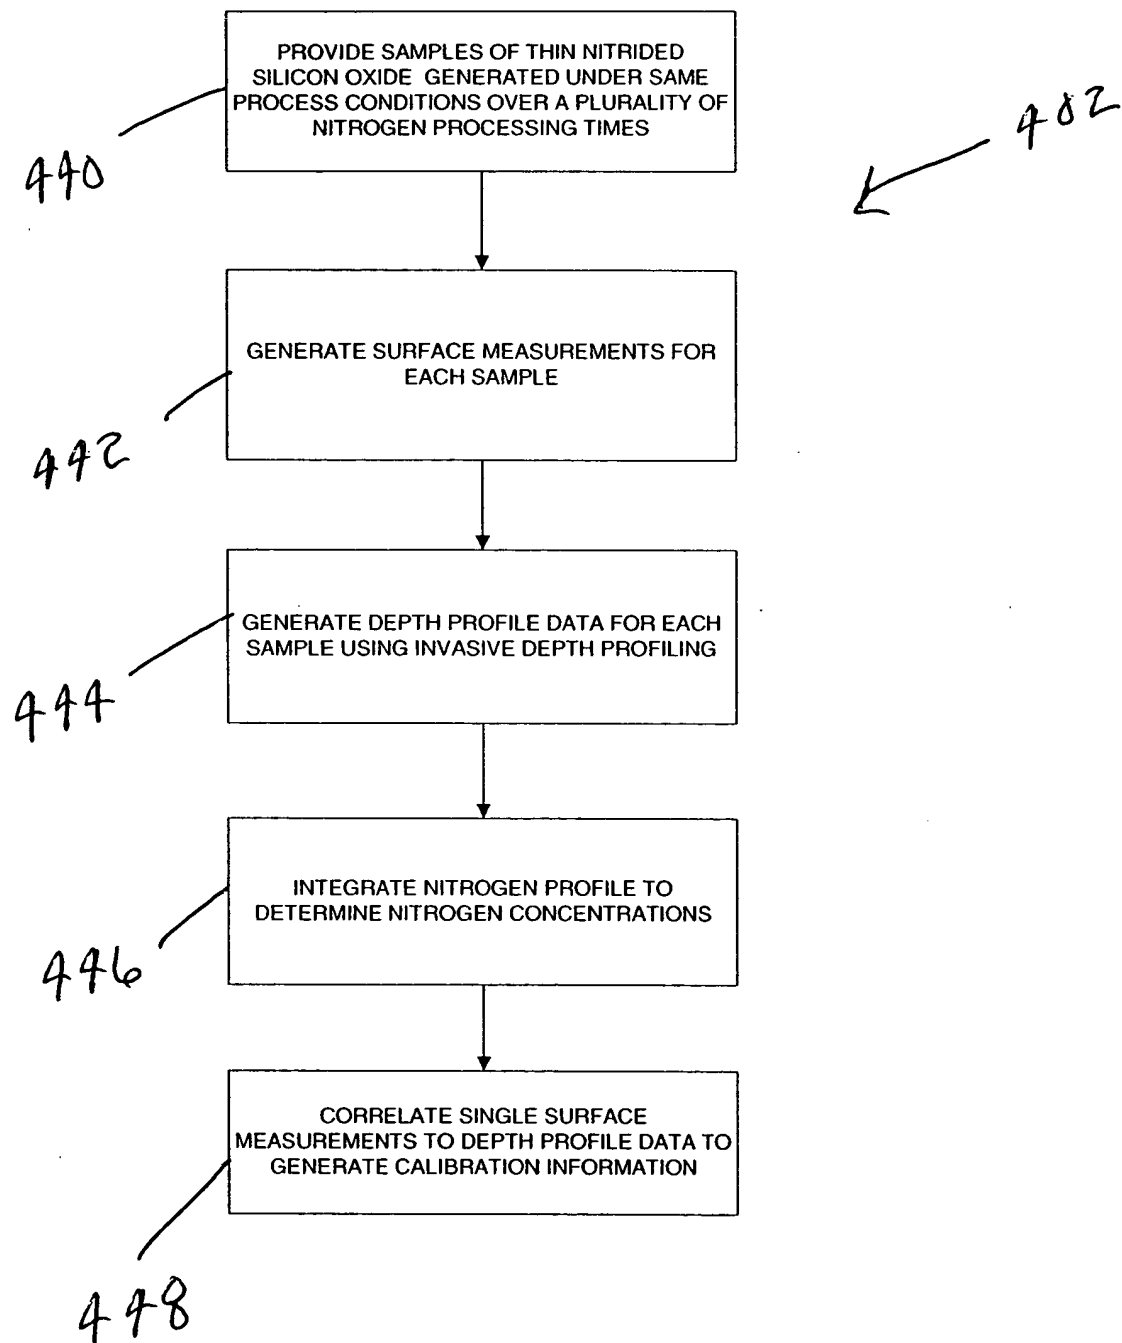

10003224-102601

FIG. 14

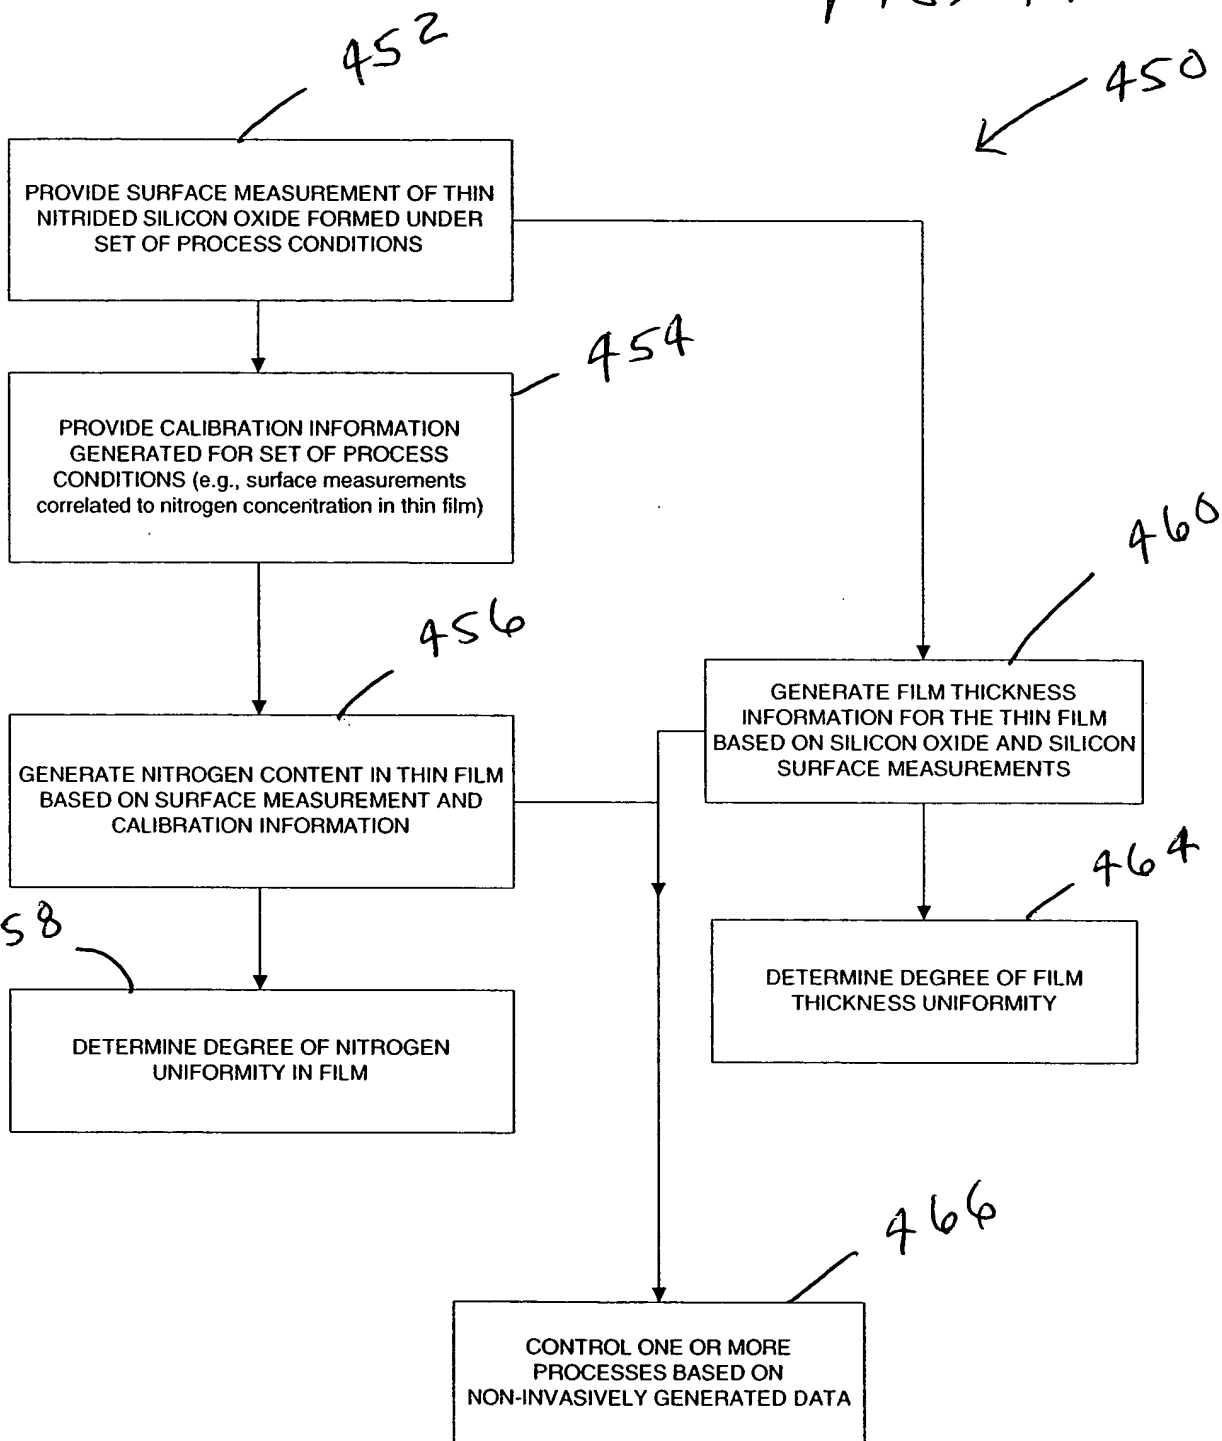

1000324-102601

FIG. 15

490 →

